

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
14 April 2005 (14.04.2005)

PCT

(10) International Publication Number
WO 2005/032373 A1

(51) International Patent Classification⁷: **A61B 6/00**

(21) International Application Number:
PCT/IB2004/051847

(22) International Filing Date:
24 September 2004 (24.09.2004)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
03103667.6 2 October 2003 (02.10.2003) EP

(71) Applicant (for DE only): **PHILIPS INTELLECTUAL
PROPERTY & STANDARDS GMBH** [DE/DE]; Stein-
damm 94, 20099 Hamburg (DE).

(71) Applicant (for AE, AG, AL, AM, AT, AU, AZ, BA, BB, BE,
BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CY, CZ,

DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM,
HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK,
LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ,
NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD,
SE, SG, SK, SL, SY, SZ, TJ, TM, TN, TR, TT, TZ, UA, UG,
UZ, VC, VN, YU, ZA, ZM, ZW only): **KONINKLIJKE
PHILIPS ELECTRONICS N. V.** [NL/NL]; Groenewoud-
seweg 1, NL-5621 BA Eindhoven (NL).


(72) Inventors; and

(75) Inventors/Applicants (for US only): **VOGTMEIER,
Gereon** [DE/DE]; c/o Philips Intellectual Property &
Standards GmbH Weissshausstr. 2, 52066 Aachen (DE).
MORALES SERRANO, Francisco [MX/DE]; c/o
Philips Intellectual Property &, Standards GmbH Weis-
shausstr. 2, 52066 Aachen (DE).

(74) Agent: **VOLMER, Georg**; Philips Intellectual Property
&, Standards GmbH Weissshausstr. 2, 52066 Aachen (DE).

[Continued on next page]

(54) Title: X-RAY UNIT

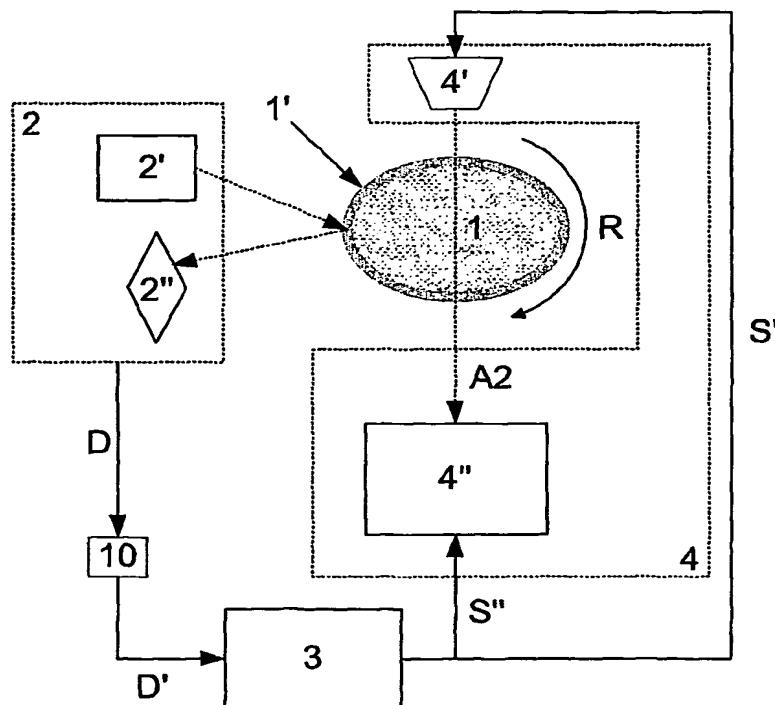

(57) Abstract: An X-ray unit according to the invention has a first arrangement (2) that is intended for the contactless and X-ray free measurement of first data of an object (1). A control unit (3) controls, on the basis of the first data of the object, a second arrangement (4) that measures X-ray data of the object by means of X-rays. With such an X-ray unit, first data 5 of the object can be obtained without using X-rays and control of the measurement of the X-ray data is made possible, with the result that, for optimum quality of the X-ray data, only a minimum X-ray dose is applied to the object.



(81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH,

GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.